GENERAL RADIO COMPANY CAMBRIDGE, MASSACHUSETTS, U. S. A.

OPERATING INSTRUCTIONS FOR

TYPE 614-A SELECTIVE AMPLIFIER

PART 1 DESCRIPTION

PURPOSE The Type 614-A Selective Amplifier is designed for producing and selecting the first ten harmonics of a 1000-cycle voltage applied to its input terminals. The instrument is particularly useful in connection with the Class C-21-H Primary Frequency Standard as it permits comparisons to be made at each multiple of 1 kc with the same accuracy as that of the primary standard. The instrument is also useful in connection with calibrations made with a cathode-ray oscillograph.

PRINCIPLE OF OPERATION The applied 1-kc voltage is impressed on a harmonic-producing tube. The

output circuit of this tube is provided with ten fixed tuned circuits, any one of which may be placed in circuit by means of the SELECTOR switch. A stage of amplification follows the tuned circuits, arranged so as to provide regeneration for sharpening the tuning. An output amplifier, with an output meter, not only raises the level of the output, but provides for essentially isolating the regenerative tube from effects of changes in load impedance.

POWER SUPPLY The Type 614-A Selective Amplifier is completely a-c operated from 115-volt 50-60 cycle mains.

PART 2 INSTALLATION

VACUUM TUBES

Install as follows:

Туре	Location (Seen from rear)
82	Left socket (4-prong)
56	3 Right sockets (5-prong)

PART 3 **OPERATION**

Throw the FIL-PLATE switch to "ON". The panel bull's-eye should light, showing that power is on. Set SELECTOR switch on the point corresponding to the multiple of 1 kc desired. Set output meter shunt at maximum (to right). Advance input control from minimum (at left) until a reading is obtained on output meter. Next advance regeneration control toward the right, reducing the input, if necessary, until the point of oscillation is almost reached. If these instructions are followed, the maximum output, consistent with the best waveform, will be obtained.

Where the best waveform is not required, considerably more output may be ob-

tained by advancing the input control or the regeneration control, or both, for maximum output voltage. If the output voltage exceeds the range of the meter, move the meter shunt toward the left.

The presence of beats on the meter. or an abnormally high output meter reading, are indications that the amplifier is oscillating and that the regeneration should be reduced by moving the regeneration control to the left.

Some readjustment of both input control and regeneration control will be required for each setting of the SELECTOR switch.

Connections for the 115-

volt 50-60 cycle supply should be made through the motor-attachment plug provided for the purpose. The 1-kc input and the harmonic output terminals are available on the front panel for temporary connections; these also appear on the multipoint connector at the rear of

the instrument for permanent connections.

CONNECTIONS

GENERAL RADIO COMPANY

PART 4 SPECIFICATIONS

Frequency Range: Each multiple of 1 kc from 1 to 10 inclusive.

Power Supply: 115 volts, 50-60 cycles.

Power Input: 25 watts.

<u>Controls:</u> Power supply ON-OFF switch: input voltage control; regeneration control; output meter shunt; harmonic selector switch.

Meters: Output meter.

1 kc <u>Tubes:</u> Supplied with instrument.

1 - 82 Rectifier 3 - 56 Amplifiers

<u>Mounting:</u> Standard 19-inch relay-rack mounting. Unit fitted with dust cover.

Accessories Supplied: See packing list.

Additional Accessories Required: None.

<u>Dimensions:</u> Panel (width) 19 x (height) 8-3/4 x (depth) 11 inches, over-all.

Net Weight: 38 pounds.

VACUUM-TUBE DATA

These data were measured on a stock model of the Type 614-A Selective Amplifier using a Weston Model 772 Analyzer. Where operating voltages and currents are obviously not critical, variations of as much as 20% from these values may be expected.

Tube	Function	Filament (60~)	Plate to Cathode	Plate Current	Grid Bias
Tl	-	2.5 volts	135 volts	3.5 ma	-7 volts
T2		2.5 volts	180 volts	5.5 ma	-8.5 volts
TЗ		2.5 volts	150 volts	2.3 ma	-9.0 volts
Τ4	Rectifier †	2.5 volts	175 volts (60~)	-	-

Type 614-A Selective Amplifier*


*No signal input. Regeneration control at zero.

+D-C output (cathode-to-ground) = 200 volts.

PATENT NOTICE

This instrument is manufactured under the following U. S. Patents and license agreements:

Patents of the American Telephone and Telegraph Company, solely for utilization in research, investigation, measurement, testing, instruction and development work in pure and applied science.

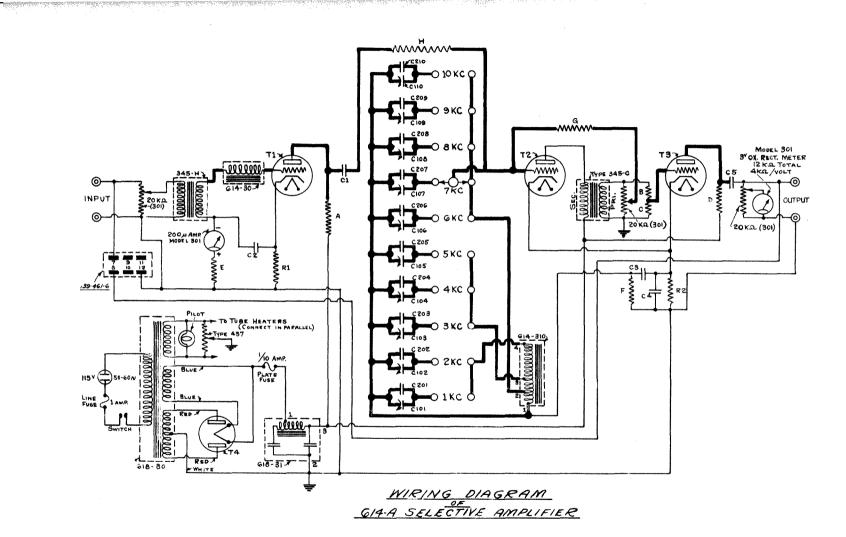

a par inference and a state of the state of a



1

GENERAL RADIO COMPANY

PARTS LIST

-

Condensers

C-1	=	0.01 uf
		1.0 µf
		1.0 µf
		1.0 uf
		0.05 µf
		1000-3000 µµf
		.0140 µf + 100 µµf
		500-1000 uuf
		.00325 µf + 25 µµf
		500-1000 uuf
C -20 3	=	.00500 µf + 25 µµf
		500-1000 µµf
C-204	=	.00245 µf + 25 µµf
C-105	=	200 - 500 µµf
C-205	=	.00165 µf ± 15 µµf
		500-1000 uuf
C-206	Ξ	.00205 µf ± 25 µµf
C-107	=	200-500 µµf
C-207	Ξ	.00150 µf + 15 µµf
		200-500 µµf
C-208	=	.00095 µf <u>+</u> 15 µµf
		200-500 µµf
		.00060 µf <u>+</u> 15 µµf
		200-500 µµf
C-210	=	.00030 µf <u>+</u> 15 µµf

Res	istors	

Α	m	20,000 Q
В	=	50,000 R
C	=	15 ,000 Ω
D	=	20,000 Ω
Е	=	10,000 Ω
F	H	50,000 Q
G	=	0.25 ΜΩ
Н	=	2 MΩ
Rl	=	2000 Ω
R2	=	1200 Ω

Tubes

Τ1	=	RCA-56
Т2	=	RCA-56
ΤЗ	=	RCA-56
T4	=	RCA-82

PACKING LIST

Attachment cord and plug
Multipoint connector
0.1-ampere fuses
1-ampere fuses

2 - Pilot lamps (2.5 volt) 1 - 82 Rectifier 3 - 56 Amplifiers

Form 404-B